

TEST REPORT

(Electronic version)



No: 200093460

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: GTQP-0440-34

ISSUE DATE: 2020-04-26

检测报告



APPLICANT: DONGGUAN FORES BIOTECHNOLOGY CO., LTD
ADDRESS: ROOM 201, NO. 1 BUILDING, NO. 5, SHIPAI INDUSTRIAL AVENUE, SHIPAI TOWN, DONGGUAN CITY, GUANGDONG PROVINCE

INFORMATION CONFIRMED BY APPLICANT:

DISPOSABLE MEDICAL FACE MASK

QUANTITY: THIRTY PIECES

MANUFACTURE'S NAME: DONGGUAN FORES BIOTECHNOLOGY CO., LTD

DATE RECEIVED/DATE TEST STARTED: 2020-04-24

CONCLUSION:

RESIDUAL ETHYLENE OXIDE M

BACTERIAL FILTRATION EFFICIENCY M


NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200072958.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

WanLi Hu ENGINEER




PAGE 1 OF 3

TEST REPORT

(Electronic version)

No:200093460

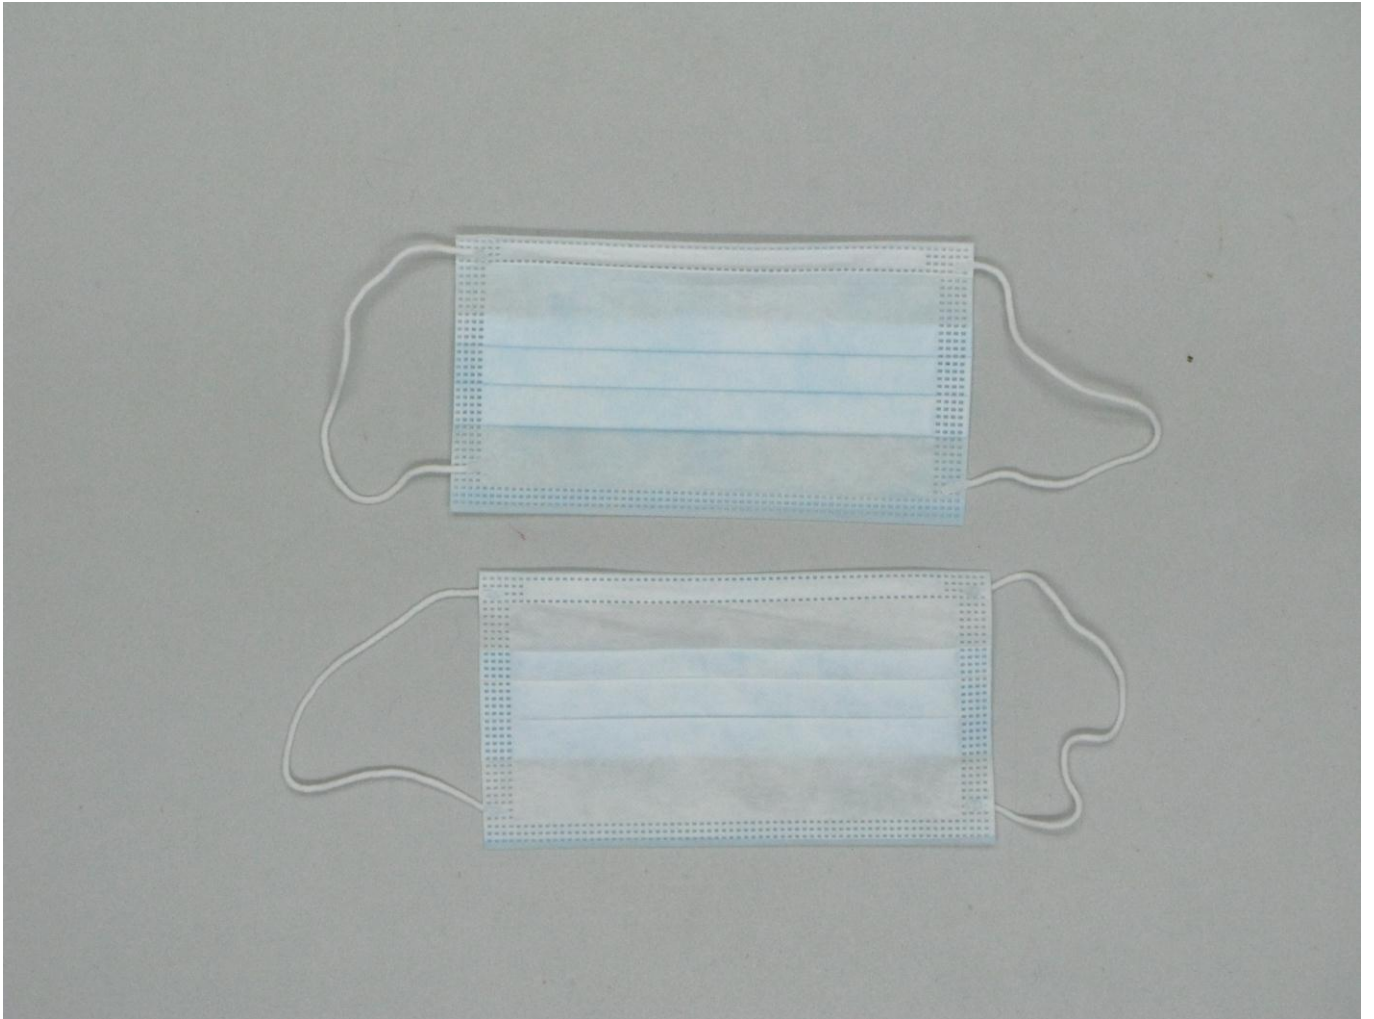

TEST REPORT

(Electronic version)

No:200093460

RESIDUAL ETHYLENE OXIDE

(GB/T 14233.1-2008)

NOT DETECTED

(DETECTION LIMIT:0.5 μg/g)

REQUIREMENT

≤10 μg/g

(YY/T 0969-2013)

BACTERIAL FILTRATION EFFICIENCY (%)

(YY 0469-2011 ANNEX B, TEST BACTERIA: STAPHYLOCOCCUS AUREUS ATCC 6538, TEST AREA: 40cm², FLOW RATE: 28.3L/min, MEAN PARTICLE SIZE: 3.0 μm, RESULT OF THE POSITIVE CONTROL: 1.9×10³ CFU, RESULT OF THE NEGATIVE CONTROL: <1CFU)

REQUIREMENT

≥95

(YY/T 0969-2013)

BFE₁ 95.4

BFE₂ 95.3

BFE₃ 95.1



—End of Report—

PAGE 3 OF 3