

## TEST REPORT

(Electronic version)



No:200099416

VERIFICATION WEBSITE: [www.gttc.net.cn](http://www.gttc.net.cn)

VERIFICATION CODE: WYNU-8046-24

ISSUE DATE:2020-04-26

二维码载报告



APPLICANT: DONGGUAN FORES BIOTECHNOLOGY CO., LTD  
ADDRESS: ROOM 201, NO. 1 BUILDING, NO. 5, SHIPAI INDUSTRIAL AVENUE, SHIPAI TOWN, DONGGUAN CITY, GUANGDONG PROVINCE

INFORMATION CONFIRMED BY APPLICANT:

DISPOSABLE FACE MASK

QIANTITY: FIFTEEN PIECES

MANUFACTURE'S NAME: DONGGUAN FORES BIOTECHNOLOGY CO., LTD

DATE RECEIVED/DATE TEST STARTED: 2020-04-25

CONCLUSION:

RESIDUAL ETHYLENE OXIDE	M
COLIFORM GROUP	M
TOTAL AMOUNT OF BACTERIAL COLONY	M
TOTAL AMOUNT OF FUNGUS COLONY	M
PSEUDOMONAS AERUGINOSA	M
STAPHYLOCOCCUS AUREUS	M
HEMOLYTIC STREPTOCOCCUS	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT  
"---" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200076578.  
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).  
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.  
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

ZiShan Guo SENIOR ENGINEER

郭子山




PAGE 1 OF 3

# TEST REPORT

(Electronic version)

No:200099416

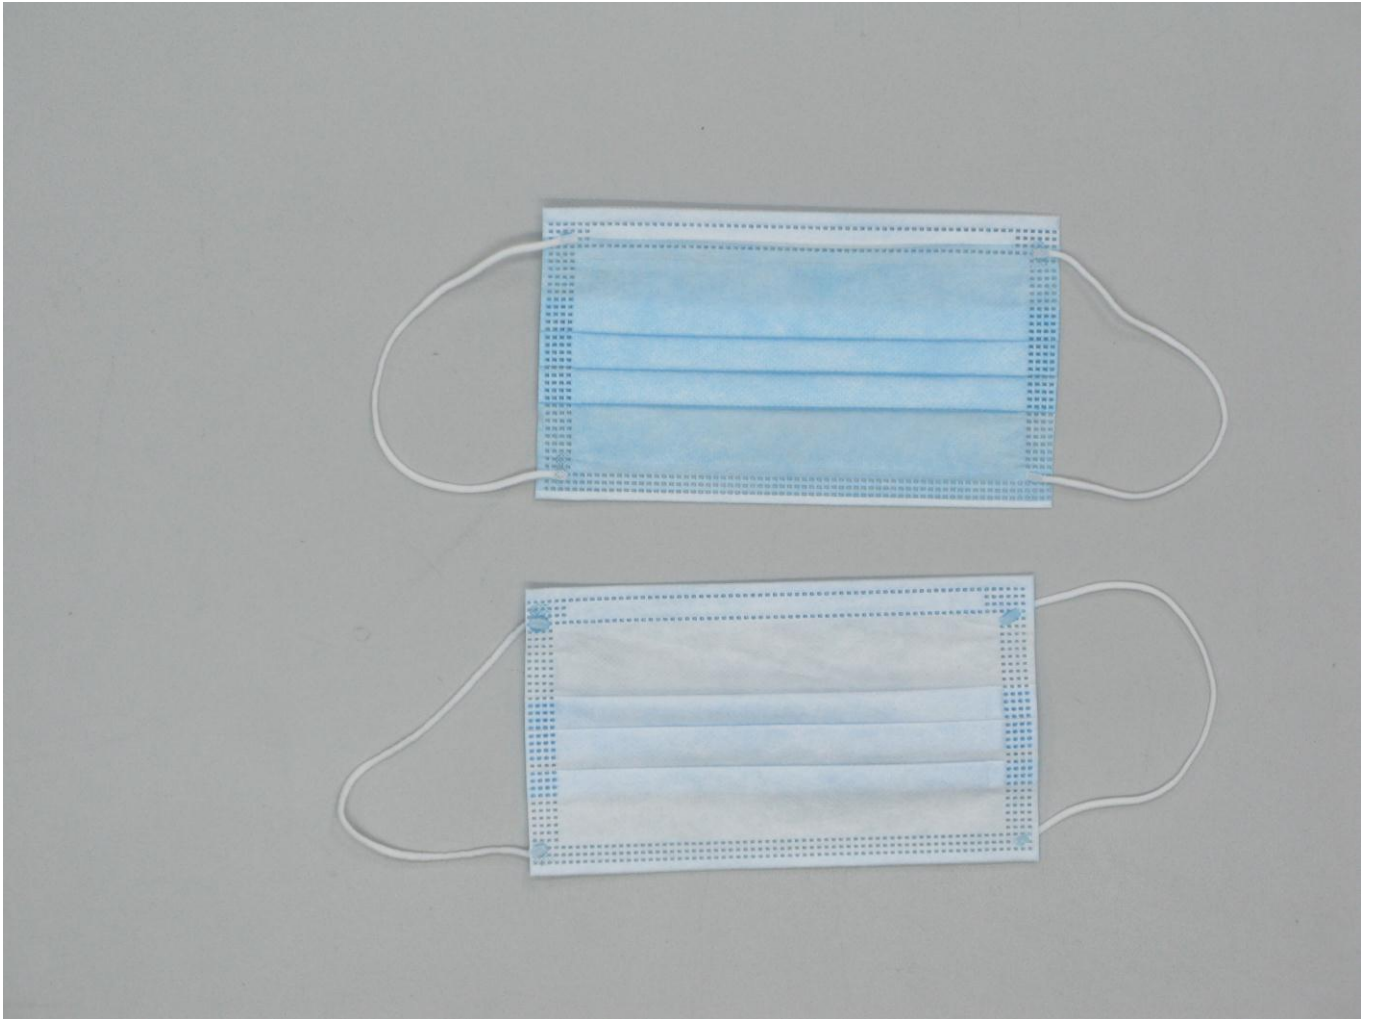

# TEST REPORT

(Electronic version)

No:200099416

---

## RESIDUAL ETHYLENE OXIDE

(GB/T 14233.1-2008)

3.6  $\mu\text{g/g}$   
(DETECTION LIMIT:0.5  $\mu\text{g/g}$ )

REQUIREMENT  
 $\leq 10 \mu\text{g/g}$   
(GB/T 32610-2016)

---

## COLIFORM GROUP

(GB 15979-2002 ANNEX B)

NOT DETECTED

REQUIREMENT  
MUST NOT BE DETECTED  
(GB/T 32610-2016)

---

## TOTAL AMOUNT OF BACTERIAL COLONY (CFU/g)

(GB 15979-2002 ANNEX B)

100

REQUIREMENT  
 $\leq 200$   
(GB/T 32610-2016)

---

## TOTAL AMOUNT OF FUNGUS COLONY (CFU/g)

(GB 15979-2002 ANNEX B)

<20

REQUIREMENT  
 $\leq 100$   
(GB/T 32610-2016)

---

## PSEUDOMONAS AERUGINOSA

(GB 15979-2002 ANNEX B)

NOT DETECTED

REQUIREMENT  
MUST NOT BE DETECTED  
(GB/T 32610-2016)

---

## STAPHYLOCOCCUS AUREUS

(GB 15979-2002 ANNEX B)

NOT DETECTED

REQUIREMENT  
MUST NOT BE DETECTED  
(GB/T 32610-2016)

---

## HEMOLYTIC STREPTOCOCCUS

(GB 15979-2002 ANNEX B)

NOT DETECTED

REQUIREMENT  
MUST NOT BE DETECTED  
(GB/T 32610-2016)

---



—End of Report—

PAGE 3 OF 3